

Figure 1. EF and IR values acquired by repetitive injection of calibration standards at different concentrations

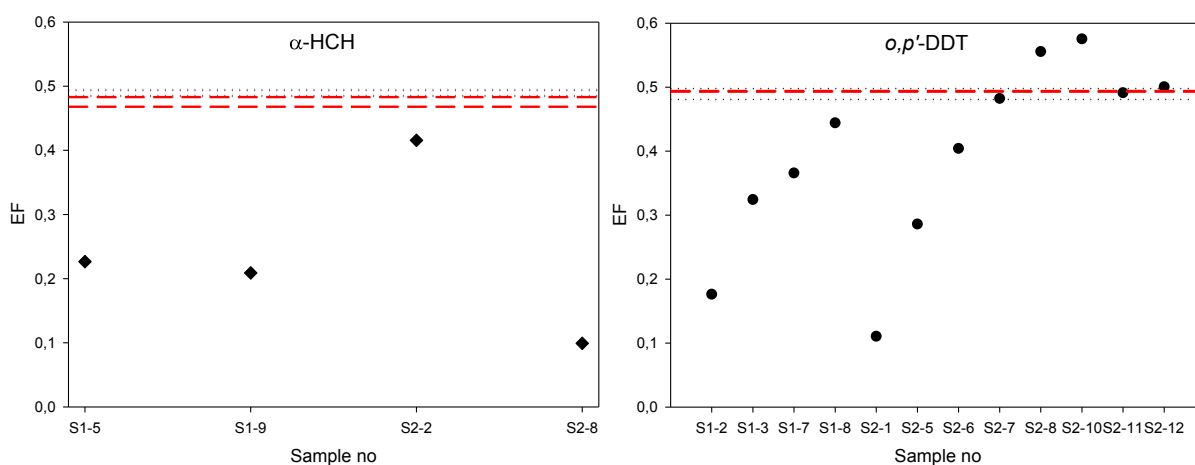


Figure 2. EF values of α -HCH and *o,p'*-DDT in samples and comparison with racemic values (black lines show considering a constant concentration and red lines show the racemic range considering concentration)

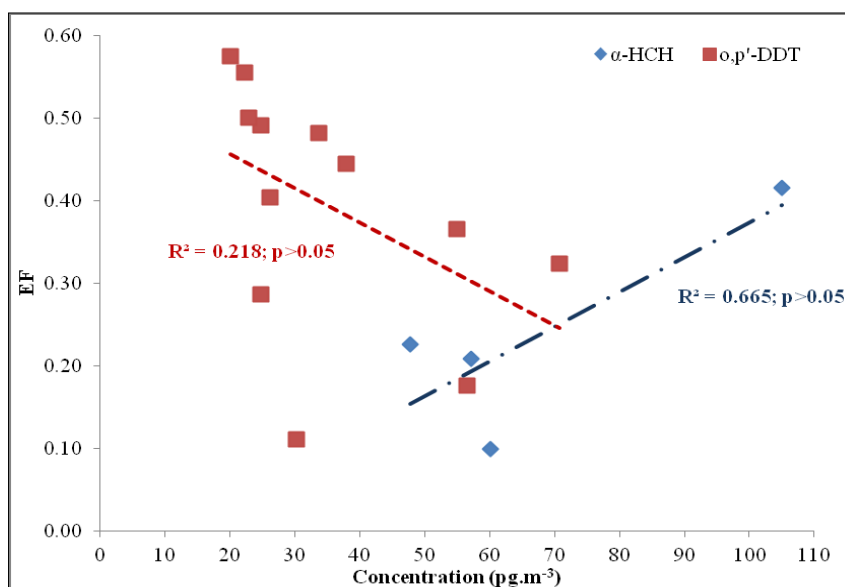


Figure 3. The relationship between EF and concentration